

EXHIBIT “A” INSTRUCTIONS

1. **Manufacturer: A-dec or Equivalent**

Three (3) Dental Operatory System Units

Request configuration (all components mounted on the dental chair)

Dental Operatory Chair: Three (3) A-dec 311 Chairs

- Formed Upholstery
- Color: Sapphire
- Two (2) position armrests (movable)
- Maximum patient weight capacity 400 pounds
- Chair base – Height adjustable
- 60% Swivel (30 degrees each side of center)
- Dual-articulating and gliding headrest
- Chair control via delivery system control pad or foot switch

System Mount: Three (3) A-dec 332 Radius system mount, chair mounting

Delivery System: Three (3) A-dec 332 Traditional Radius Delivery System

- Radius mount to dental chair
- Traditional delivery system configuration
- Control block three (3) position
- Handpiece holder positions – four (4) + air/water syringe
- Position two (2), three (3), and four (4) – four (4) hole tubing (no fiberoptics)
- Standard touch pad with delivery system (with chair controls)
- With Tray for instruments
- Foot control: Disc foot control

Assistant’s Holder System: Three (3) A-dec 351 Radius ASST Radius mount to dental chair

- Four (4) position holder
 - a. Air/Water Syringe and three (3) other holders (including one (1) saliva ejector, two (2) high volume evacuator (HVE))

- Assistant touch pad with chair controls

Cuspidor: None (0)

Dental Light: Three (3) A-dec 372L LED Dental Light, Radius Mount

- Radius mount to dental chair
- LED Light
- Minimum four (4) bright white LED
- Touchpad function for light
- Composite Mode
- Rotational axes – three (3) axis

Monitor: None (0)

2. **Manufacturer: A-dec or Equivalent**

One (1) Dental Chair with one (1) LED Mounted Light

Requested configuration (LED light mounted on the dental chair)

Dental Operatory Chair: One (1) A-dec 311 Chair

- Formed Upholstery
- Color: Sapphire
- Two position armrests (movable)
- Maximum patient weight capacity 400 pounds
- Chair base – Height adjustable
- 60% Swivel (30 degrees each side of center)
- Dual-articulating and gliding headrest
- Chair control via delivery system control pad or foot switch

Dental Light: One (1) A-dec 372L LED Dental Light, Radius Mount

- Radius mount to dental chair
- LED Light
- Minimum four (4) bright white LED
- Touchpad function for light

- Composite Mode
- Rotational axes – three (3) axis

3. Manufacturer: A-dec or Equivalent

One (1) Stand-alone Dental Delivery System Cart

Requested configuration

Cart Delivery System: One (1) A-dec 343 Pro cart

- Control block three (3) position
- Handpiece holder positions – four (4) + syringe
- Position two (2), three (3), and four (4) – four (4) hole tubing
- Standard touch pad with delivery system (with chair controls)
- With Tray for instruments
- Assistant Arm holder - Air/water syringe and three (3) other holders (including one (1) saliva ejector, two (2) HVE)

4. Dental Operatory Unit Manufacturer’s Warranty – Parts

Requirement: Ten (10) year Manufacturer Warranty for parts covering dental chairs, delivery of dental operatory system units, and lights.

5. Dental Operatory System Unit Extended Warranty – Service, Repair, and Labor (excluding parts)

Requirement: The Contractor shall provide a ten (10) year extended warranty covering service, labor, and repair for all four (4) dental operatory system units purchased.


*Images of the HCDSB’s Dental Clinic Operatory Rooms and Existing Dental Operatory System Units to be Replaced are listed below:

Lanakila Health Center, Dental Clinic ~ Operatory #1






Leeward Health Center, Dental Clinic ~ Operatory #1

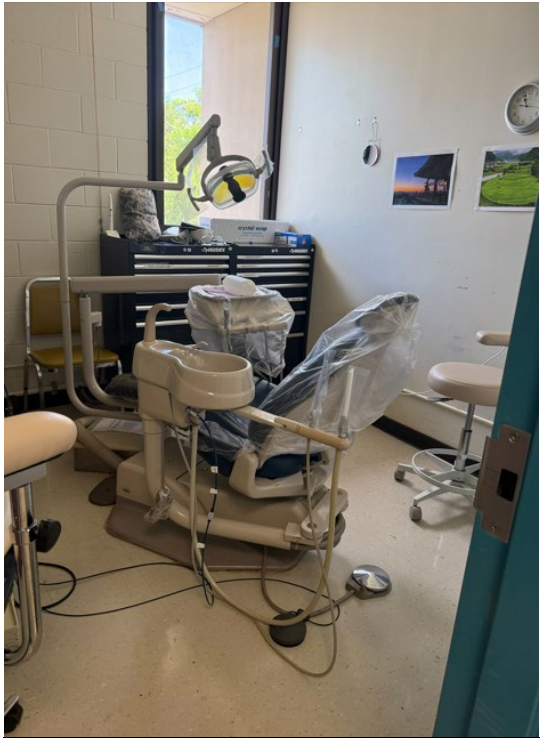



Leeward Health Center, Dental Clinic ~ Operatory #2



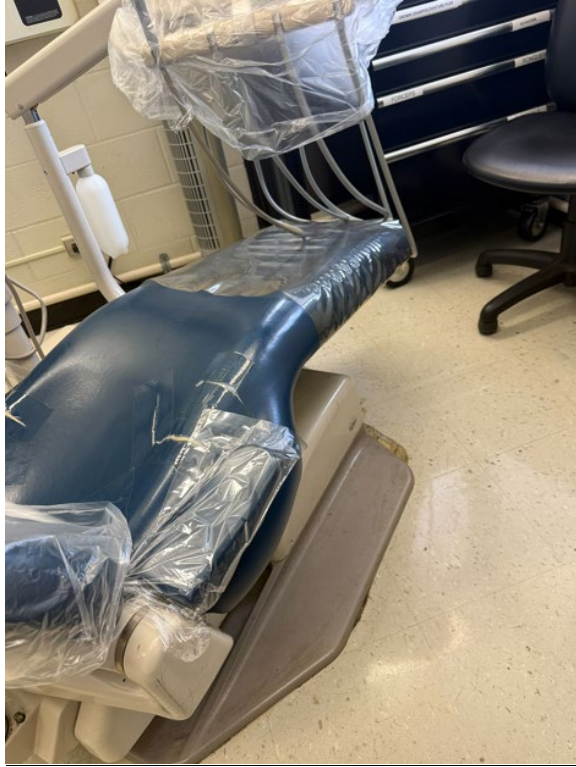

Windward Health Center, Dental Clinic ~ Operatory #2



